

## CALIBRATION CERTIFICATE

| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
|----------------|----------------------|------------------|-------------------|-----------|
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1447 | 24.Oct.2025       | 01 of 01  |

M/s Apex Buildsys Limited.

Plot No - D3, MIDC Industrial Area,  
Umred, Dist-Nagpur.

## CUSTOMER REFERENCE

SRF No : ACIPL/JC/25-26/883

Gate Pass No. : -

Date of Receipt : 18.Oct.2025

Order Inward No. ACIPL/25-ISO/10/883/A-132

Location of Calibration : Onsite

## 01 Description &amp; Identification

UUC : Analog Welding Machine  
 Make : Panasonic  
 Model No. : KRII350  
 Serial No. : 1020900369  
 ID. No. : PANA/WM-01  
 Range : 0 to 400 Amp & 0 to 75 Volts  
 Least Count : 20 Amp & 2 Volts

## 02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION

| SI NO. | DESCRIPTION | SR.NO.     | TRACEABILITY   | VALIDITY    | CERTIFICATE NO.  |
|--------|-------------|------------|----------------|-------------|------------------|
| 01     | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

## 03 Calibration Procedure reference

AE / DFT / 02 - CM/ET/06/08

## 04 Environmental Conditions

Temperature at 27.5 °C &amp; 45 to 75 % RH

## 05 Calibration Result in Volts. (Observed value is mean of Five reading)

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 20    | 19.85             | 20             | 0.15      |
| 02     | 40    | 39.5              | 40             | 0.5       |
| 03     | 50    | 49.2              | 50             | 0.8       |
| 04     | 70    | 69.2              | 70             | 0.8       |

## Calibration Result in Amp. (Observed value is mean of Five reading)

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 100   | 100.2             | 100            | -0.2      |
| 03     | 200   | 200.8             | 200            | -0.8      |
| 04     | 300   | 301.2             | 300            | -1.2      |


## 06 Remarks

01. This certificate issued as per customer requirement.

02. UUC = Unit Under Calibration.

03. The Standards used for calibration are traceable to National / International Standard through accredited Laboratories.

\*\*\*\* End of Certificate \*\*\*\*

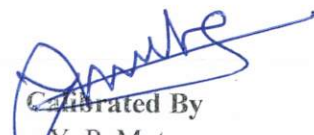  
 Calibrated By  
 Y. P. Mute  
 Calibration Engg.



  
 Authorised By  
 A. S. Choudhari  
 Quality Manager

AE/RFT-50

## CALIBRATION CERTIFICATE

| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
|----------------|----------------------|------------------|-------------------|-----------|
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1448 | 24.Oct.2025       | 01 of 01  |

M/s Apex Buildsys Limited.

Plot No - D3, MIDC Industrial Area,

Umred, Dist-Nagpur.

## CUSTOMER REFERENCE

SRF No : ACIPL/JC/25-26/883

Gate Pass No. : -

Date of Receipt : 18.Oct.2025

Order Inward No. ACIPL/25-ISO/10/883/A-133

Location of Calibration : Onsite

## 01 Description &amp; Identification

UUC : Analog Welding Machine

Make : Panasonic

Model No. : YD-500KR2

Serial No. : D10623O0017

ID. No. : MIG-343

Range : 0 to 600 Amp &amp; 0 to 75 Volts

Least Count : 20 Amp &amp; 5 Volts

## 02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION

| SI NO. | DESCRIPTION | SR.NO.     | TRACEABILITY   | VALIDITY    | CERTIFICATE NO.  |
|--------|-------------|------------|----------------|-------------|------------------|
| 01     | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

## 03 Calibration Procedure reference

AE / DFT / 02 - CM/ET/06/08

## 04 Environmental Conditions

Temperature at 27.5 °C &amp; 45 to 75 % RH

## 05 Calibration Result in Volts. (Observed value is mean of Five reading)

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 20    | 19.85             | 20             | 0.15      |
| 02     | 40    | 39.5              | 40             | 0.5       |
| 03     | 50    | 49.2              | 50             | 0.8       |
| 04     | 70    | 69.2              | 70             | 0.8       |

## Calibration Result in Amp. (Observed value is mean of Five reading)

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 100   | 99.8              | 100            | 0.2       |
| 02     | 200   | 199.4             | 200            | 0.6       |
| 03     | 300   | 298.8             | 300            | 1.2       |
| 04     | 500   | 499               | 500            | 1         |


## 06 Remarks

01.This certificate issued as per customer requirment.

02.UUC = Unit Under Calibration.

03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.

\*\*\*\* End of Certificate \*\*\*\*




Calibrated By  
Y. P. Mute  
Calibration Engg.




Authorised By  
A. S. Choudhari  
Quality Manager

AE/RFT-50

## CALIBRATION CERTIFICATE
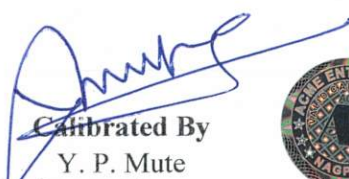
|                                                                                                                                         |                                     |                                                                                                                                                                                                      |                                  |                       |                  |
|-----------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------|-----------------------|------------------|
| Calibration On<br>18.Oct.2025                                                                                                           | Next Calibration Due<br>17.Oct.2026 | Certificate No.<br>AE/WM/25/10/1449                                                                                                                                                                  | Certi. Issue Date<br>24.Oct.2025 | Sheet No.<br>01 of 01 |                  |
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur.                                         |                                     | CUSTOMER REFERENCE                                                                                                                                                                                   |                                  |                       |                  |
|                                                                                                                                         |                                     | SRF No : ACIPL/JC/25-26/883                                                                                                                                                                          |                                  |                       |                  |
|                                                                                                                                         |                                     | Gate Pass No. : -                                                                                                                                                                                    |                                  |                       |                  |
|                                                                                                                                         |                                     | Date of Receipt : 18.Oct.2025                                                                                                                                                                        |                                  |                       |                  |
| Order Inward No.                                                                                                                        | ACIPL/25-ISO/10/883/A-134           | Location of Calibration : Onsite                                                                                                                                                                     |                                  |                       |                  |
| 01 Description & Identification :                                                                                                       |                                     | UUC : Analog Welding Machine<br>Make : Panasonic<br>Model No. : YD-500KR2<br>Serial No. : D10623O0113<br>ID. No. : MIG-335<br>Range : 0 to 600 Amp & 0 to 75 Volts<br>Least Count : 20 Amp & 5 Volts |                                  |                       |                  |
| 02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION                                                                      |                                     |                                                                                                                                                                                                      |                                  |                       |                  |
| SI NO.                                                                                                                                  | DESCRIPTION                         | SR.NO.                                                                                                                                                                                               | TRACEBILITY                      | VALIDITY              | CERTIFICATE NO.  |
| 01                                                                                                                                      | Clamp Meter                         | 2408077674                                                                                                                                                                                           | NABL CC - 2632                   | 19.May.2026           | AE/CC/25-26/3349 |
| 03 Calibration Procedure reference                                                                                                      |                                     | AE / DFT / 02 - CM/ET/06/08                                                                                                                                                                          |                                  |                       |                  |
| 04 Environmental Conditions                                                                                                             |                                     | Temperature at 27.5 °C & 45 to 75 % RH                                                                                                                                                               |                                  |                       |                  |
| 05 Calibration Result in Volts. (Observed value is mean of Five reading)                                                                |                                     |                                                                                                                                                                                                      |                                  |                       |                  |
| SI No.                                                                                                                                  | Range                               | Observe on Master                                                                                                                                                                                    | Observe on UUC                   | Deviation             |                  |
| 01                                                                                                                                      | 20                                  | 20.25                                                                                                                                                                                                | 20                               | -0.25                 |                  |
| 02                                                                                                                                      | 40                                  | 40.3                                                                                                                                                                                                 | 40                               | -0.3                  |                  |
| 03                                                                                                                                      | 50                                  | 50.5                                                                                                                                                                                                 | 50                               | -0.5                  |                  |
| 04                                                                                                                                      | 70                                  | 70.8                                                                                                                                                                                                 | 70                               | -0.8                  |                  |
| Calibration Result in Amp. (Observed value is mean of Five reading)                                                                     |                                     |                                                                                                                                                                                                      |                                  |                       |                  |
| SI No.                                                                                                                                  | Range                               | Observe on Master                                                                                                                                                                                    | Observe on UUC                   | Deviation             |                  |
| 01                                                                                                                                      | 100                                 | 100.3                                                                                                                                                                                                | 100                              | -0.3                  |                  |
| 02                                                                                                                                      | 200                                 | 200.8                                                                                                                                                                                                | 200                              | -0.8                  |                  |
| 03                                                                                                                                      | 300                                 | 300.5                                                                                                                                                                                                | 300                              | -0.5                  |                  |
| 04                                                                                                                                      | 500                                 | 501                                                                                                                                                                                                  | 500                              | -1                    |                  |
| 06 Remarks                                                                                                                              |                                     |                                                                                                                                                                                                      |                                  |                       |                  |
| 01.This certificate issued as per customer requirment.                                                                                  |                                     |                                                                                                                                                                                                      |                                  |                       |                  |
| 02.UUC = Unit Under Calibration.                                                                                                        |                                     |                                                                                                                                                                                                      |                                  |                       |                  |
| 03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.                |                                     |                                                                                                                                                                                                      |                                  |                       |                  |
| **** End of Certificate ****                                                                                                            |                                     |                                                                                                                                                                                                      |                                  |                       |                  |
| <br>Calibrated By<br>Y. P. Mute<br>Calibration Engg. |                                     |                                                                                                                   |                                  |                       |                  |
|                                                                                                                                         |                                     |                                                                                                                 |                                  |                       |                  |
|                                                                                                                                         |                                     | Authorised By<br>A. S. Choudhari<br>Quality Manager                                                                                                                                                  |                                  |                       |                  |
| AE/RFT-50                                                                                                                               |                                     |                                                                                                                                                                                                      |                                  |                       |                  |

## CALIBRATION CERTIFICATE

| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
|----------------|----------------------|------------------|-------------------|-----------|
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1450 | 24.Oct.2025       | 01 of 01  |

M/s Apex Buildsys Limited.

Plot No - D3, MIDC Industrial Area,

Umred, Dist-Nagpur.

## CUSTOMER REFERENCE

SRF No : ACIPL/JC/25-26/883

Gate Pass No. : -

Date of Receipt : 18.Oct.2025

Order Inward No. ACIPL/25-ISO/10/883/A-135

Location of Calibration : Onsite

## 01 Description &amp; Identification

UUC : Analog Welding Machine

Make : Panasonic

Model No. : KRII350

Serial No. : 10209Y0296

ID. No. : MIG-344

Range : 0 to 400 Amp &amp; 0 to 75 Volts

Least Count : 20 Amp &amp; 2 Volts

## 02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION

| SI NO. | DESCRIPTION | SR.NO.     | TRACEABILITY   | VALIDITY    | CERTIFICATE NO.  |
|--------|-------------|------------|----------------|-------------|------------------|
| 01     | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

## 03 Calibration Procedure reference

AE / DFT / 02 - CM/ET/06/08

## 04 Environmental Conditions

Temperature at 27.5 °C &amp; 45 to 75 % RH

## 05 Calibration Result in Volts. (Observed value is mean of Five reading)

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 20    | 19.93             | 20             | 0.07      |
| 02     | 40    | 39.8              | 40             | 0.2       |
| 03     | 50    | 49.5              | 50             | 0.5       |
| 04     | 70    | 69.5              | 70             | 0.5       |

## Calibration Result in Amp. (Observed value is mean of Five reading)

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 100   | 100.3             | 100            | -0.3      |
| 03     | 200   | 201.2             | 200            | -1.2      |
| 04     | 300   | 301.8             | 300            | -1.8      |


## 06 Remarks

01.This certificate issued as per customer requirment.

02.UUC = Unit Under Calibration.

03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.

\*\*\*\* End of Certificate \*\*\*\*

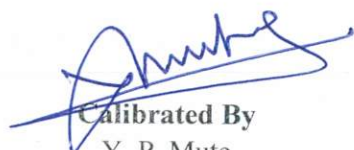

Calibrated By  
Y. P. Mute  
Calibration Engg.




Authorised By  
A. S. Choudhari  
Quality Manager

AE/RFT-50

## CALIBRATION CERTIFICATE

| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
|----------------|----------------------|------------------|-------------------|-----------|
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1451 | 24.Oct.2025       | 01 of 01  |

M/s Apex Buildsys Limited.

Plot No - D3, MIDC Industrial Area,  
Umred, Dist-Nagpur.

## CUSTOMER REFERENCE

SRF No : ACIPL/JC/25-26/883

Gate Pass No. : -

Date of Receipt : 18.Oct.2025

Order Inward No. ACIPL/25-ISO/10/883/A-136

Location of Calibration : Onsite

## 01 Description &amp; Identification :

UUC : Analog Welding Machine

Make : Panasonic

Model No. : YD-500KR2

Serial No. : D10623G0227

ID. No. : MIG-338

Range : 0 to 600 Amp &amp; 0 to 75 Volts

Least Count : 20 Amp &amp; 5 Volts

## 02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION

| SI NO. | DESCRIPTION | SR.NO.     | TRACEABILITY   | VALIDITY    | CERTIFICATE NO.  |
|--------|-------------|------------|----------------|-------------|------------------|
| 01     | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

## 03 Calibration Procedure reference

AE / DFT / 02 - CM/ET/06/08

## 04 Environmental Conditions

Temperature at 27.5 °C &amp; 45 to 75 % RH

## 05 Calibration Result in Volts. (Observed value is mean of Five reading)

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 20    | 20.45             | 20             | -0.45     |
| 02     | 40    | 40.8              | 40             | -0.8      |
| 03     | 50    | 51.3              | 50             | -1.3      |
| 04     | 70    | 71.5              | 70             | -1.5      |

## Calibration Result in Amp. (Observed value is mean of Five reading)

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 100   | 101.2             | 100            | -1.2      |
| 02     | 200   | 201.5             | 200            | -1.5      |
| 03     | 300   | 298.7             | 300            | 1.3       |
| 04     | 500   | 498               | 500            | 2         |


## 06 Remarks

01.This certificate issued as per customer requirment.

02.UUC = Unit Under Calibration.

03.The Standards used for calibration are tracebel to National / International Standard through  
accredited Laboratories.

\*\*\*\* End of Certificate \*\*\*\*




Calibrated By  
Y. P. Mute  
Calibration Engg.





Authorised By  
A. S. Choudhari  
Quality Manager

AE/RFT-50

## CALIBRATION CERTIFICATE

|                                                                                                                                         |                                     |                                                                                                                                                                                                  |                                                                                                                                              |                       |                  |
|-----------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------|-----------------------|------------------|
| Calibration On<br>18.Oct.2025                                                                                                           | Next Calibration Due<br>17.Oct.2026 | Certificate No.<br>AE/WM/25/10/1452                                                                                                                                                              | Certi. Issue Date<br>24.Oct.2025                                                                                                             | Sheet No.<br>01 of 01 |                  |
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur.                                         |                                     | <b>CUSTOMER REFERENCE</b>                                                                                                                                                                        |                                                                                                                                              |                       |                  |
|                                                                                                                                         |                                     | SRF No : ACIPL/JC/25-26/883                                                                                                                                                                      |                                                                                                                                              |                       |                  |
|                                                                                                                                         |                                     | Gate Pass No. : -                                                                                                                                                                                |                                                                                                                                              |                       |                  |
|                                                                                                                                         |                                     | Date of Receipt : 18.Oct.2025                                                                                                                                                                    |                                                                                                                                              |                       |                  |
| Order Inward No.                                                                                                                        | ACIPL/25-ISO/10/883/A-137           | Location of Calibration                                                                                                                                                                          | : Onsite                                                                                                                                     |                       |                  |
| 01 Description & Identification :                                                                                                       |                                     | UUC : Analog Welding Machine<br>Make : Panasonic<br>Model No. : KRII-500<br>Serial No. : 10308E1636<br>ID. No. : AW-06<br>Range : 0 to 400 Amp & 0 to 75 Volts<br>Least Count : 20 Amp & 2 Volts |                                                                                                                                              |                       |                  |
| 02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION                                                                      |                                     |                                                                                                                                                                                                  |                                                                                                                                              |                       |                  |
| SI NO.                                                                                                                                  | DESCRIPTION                         | SR.NO.                                                                                                                                                                                           | TRACEABILITY                                                                                                                                 | VALIDITY              | CERTIFICATE NO.  |
| 01                                                                                                                                      | Clamp Meter                         | 2408077674                                                                                                                                                                                       | NABL CC - 2632                                                                                                                               | 19.May.2026           | AE/CC/25-26/3349 |
| 03 Calibration Procedure reference                                                                                                      |                                     | AE / DFT / 02 - CM/ET/06/08                                                                                                                                                                      |                                                                                                                                              |                       |                  |
| 04 Environmental Conditions                                                                                                             |                                     | Temperature at 27.5 °C & 45 to 75 % RH                                                                                                                                                           |                                                                                                                                              |                       |                  |
| 05 Calibration Result in Volts. (Observed value is mean of Five reading)                                                                |                                     |                                                                                                                                                                                                  |                                                                                                                                              |                       |                  |
| SI No.                                                                                                                                  | Range                               | Observe on Master                                                                                                                                                                                | Observe on UUC                                                                                                                               | Deviation             |                  |
| 01                                                                                                                                      | 20                                  | 20.5                                                                                                                                                                                             | 20                                                                                                                                           | -0.5                  |                  |
| 02                                                                                                                                      | 50                                  | 50.7                                                                                                                                                                                             | 50                                                                                                                                           | -0.7                  |                  |
| 03                                                                                                                                      | 70                                  | 70.9                                                                                                                                                                                             | 72                                                                                                                                           | 1.1                   |                  |
| Calibration Result in Amp. (Observed value is mean of Five reading)                                                                     |                                     |                                                                                                                                                                                                  |                                                                                                                                              |                       |                  |
| SI No.                                                                                                                                  | Range                               | Observe on Master                                                                                                                                                                                | Observe on UUC                                                                                                                               | Deviation             |                  |
| 01                                                                                                                                      | 100                                 | 100.5                                                                                                                                                                                            | 100                                                                                                                                          | -0.5                  |                  |
| 02                                                                                                                                      | 200                                 | 201.2                                                                                                                                                                                            | 200                                                                                                                                          | -1.2                  |                  |
| 03                                                                                                                                      | 300                                 | 351.3                                                                                                                                                                                            | 350                                                                                                                                          | -1.3                  |                  |
| 06 Remarks                                                                                                                              |                                     |                                                                                                                                                                                                  |                                                                                                                                              |                       |                  |
| 01.This certificate issued as per customer requirment.                                                                                  |                                     |                                                                                                                                                                                                  |                                                                                                                                              |                       |                  |
| 02.UUC = Unit Under Calibration.                                                                                                        |                                     |                                                                                                                                                                                                  |                                                                                                                                              |                       |                  |
| 03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.                |                                     |                                                                                                                                                                                                  |                                                                                                                                              |                       |                  |
| **** End of Certificate ****                                                                                                            |                                     |                                                                                                                                                                                                  |                                                                                                                                              |                       |                  |
| <br>Calibrated By<br>Y. P. Mute<br>Calibration Engg. |                                     |                                                                                                               | <br>Authorised By<br>A. S. Choudhari<br>Quality Manager |                       |                  |
| AE/RFT-50                                                                                                                               |                                     |                                                                                                                                                                                                  |                                                                                                                                              |                       |                  |

## CALIBRATION CERTIFICATE

|                                                                                                                                         |                                     |                                                                                                                                                                                                      |                                                                                                                                              |                       |
|-----------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------|-----------------------|
| Calibration On<br>18.Oct.2025                                                                                                           | Next Calibration Due<br>17.Oct.2026 | Certificate No.<br>AE/WM/25/10/1453                                                                                                                                                                  | Certi. Issue Date<br>24.Oct.2025                                                                                                             | Sheet No.<br>01 of 01 |
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur.                                         |                                     | <b>CUSTOMER REFERENCE</b><br>SRF No : ACIPL/JC/25-26/883<br>Gate Pass No. : -<br>Date of Receipt : 18.Oct.2025                                                                                       |                                                                                                                                              |                       |
| Order Inward No.                                                                                                                        | ACIPL/25-ISO/10/883/A-138           | Location of Calibration : Onsite                                                                                                                                                                     |                                                                                                                                              |                       |
| 01 Description & Identification :                                                                                                       |                                     | UUC : Analog Welding Machine<br>Make : Panasonic<br>Model No. : YD-500KR2<br>Serial No. : D10623G0226<br>ID. No. : MIG-324<br>Range : 0 to 600 Amp & 0 to 75 Volts<br>Least Count : 20 Amp & 5 Volts |                                                                                                                                              |                       |
| 02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION                                                                      |                                     |                                                                                                                                                                                                      |                                                                                                                                              |                       |
| SI NO.                                                                                                                                  | DESCRIPTION                         | SR.NO.                                                                                                                                                                                               | TRACEABILITY                                                                                                                                 | VALIDITY              |
| 01                                                                                                                                      | Clamp Meter                         | 2408077674                                                                                                                                                                                           | NABL CC - 2632                                                                                                                               | 19.May.2026           |
| 03 Calibration Procedure reference                                                                                                      |                                     | AE / DFT / 02 - CM/ET/06/08                                                                                                                                                                          |                                                                                                                                              |                       |
| 04 Environmental Conditions                                                                                                             |                                     | Temperature at 27.5 °C & 45 to 75 % RH                                                                                                                                                               |                                                                                                                                              |                       |
| 05 Calibration Result in Volts. (Observed value is mean of Five reading)                                                                |                                     |                                                                                                                                                                                                      |                                                                                                                                              |                       |
| SI No.                                                                                                                                  | Range                               | Observe on Master                                                                                                                                                                                    | Observe on UUC                                                                                                                               | Deviation             |
| 01                                                                                                                                      | 20                                  | 20.32                                                                                                                                                                                                | 20                                                                                                                                           | -0.32                 |
| 02                                                                                                                                      | 40                                  | 40.5                                                                                                                                                                                                 | 40                                                                                                                                           | -0.5                  |
| 03                                                                                                                                      | 50                                  | 50.8                                                                                                                                                                                                 | 50                                                                                                                                           | -0.8                  |
| 04                                                                                                                                      | 70                                  | 70.8                                                                                                                                                                                                 | 70                                                                                                                                           | -0.8                  |
| Calibration Result in Amp. (Observed value is mean of Five reading)                                                                     |                                     |                                                                                                                                                                                                      |                                                                                                                                              |                       |
| SI No.                                                                                                                                  | Range                               | Observe on Master                                                                                                                                                                                    | Observe on UUC                                                                                                                               | Deviation             |
| 01                                                                                                                                      | 100                                 | 100.5                                                                                                                                                                                                | 100                                                                                                                                          | -0.5                  |
| 02                                                                                                                                      | 200                                 | 200.5                                                                                                                                                                                                | 200                                                                                                                                          | -0.5                  |
| 03                                                                                                                                      | 300                                 | 300.8                                                                                                                                                                                                | 300                                                                                                                                          | -0.8                  |
| 04                                                                                                                                      | 500                                 | 501                                                                                                                                                                                                  | 500                                                                                                                                          | -1                    |
| 06 Remarks                                                                                                                              |                                     |                                                                                                                                                                                                      |                                                                                                                                              |                       |
| 01.This certificate issued as per customer requirment.                                                                                  |                                     |                                                                                                                                                                                                      |                                                                                                                                              |                       |
| 02.UUC = Unit Under Calibration.                                                                                                        |                                     |                                                                                                                                                                                                      |                                                                                                                                              |                       |
| 03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.                |                                     |                                                                                                                                                                                                      |                                                                                                                                              |                       |
| **** End of Certificate ****                                                                                                            |                                     |                                                                                                                                                                                                      |                                                                                                                                              |                       |
| <br>Calibrated By<br>Y. P. Mute<br>Calibration Engg. |                                     |                                                                                                                   | <br>Authorised By<br>A. S. Choudhari<br>Quality Manager |                       |
| AE/RFT-50                                                                                                                               |                                     |                                                                                                                                                                                                      |                                                                                                                                              |                       |

## CALIBRATION CERTIFICATE

|                |                      |                  |                   |           |
|----------------|----------------------|------------------|-------------------|-----------|
| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1454 | 24.Oct.2025       | 01 of 01  |

|                                                                                                 |                           |                         |          |
|-------------------------------------------------------------------------------------------------|---------------------------|-------------------------|----------|
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur. | <b>CUSTOMER REFERENCE</b> |                         |          |
|                                                                                                 | SRF No                    | : ACIPL/JC/25-26/883    |          |
|                                                                                                 | Gate Pass No.             | : -                     |          |
|                                                                                                 | Date of Receipt           | : 18.Oct.2025           |          |
| Order Inward No.                                                                                | ACIPL/25-ISO/10/883/A-139 | Location of Calibration | : Onsite |

**01 Description & Identification :**

|             |                                |
|-------------|--------------------------------|
| UUC         | : Analog Welding Machine       |
| Make        | : Panasonic                    |
| Model No.   | : YD-500KR2                    |
| Serial No.  | : D10623I0418                  |
| ID. No.     | : MIG-339                      |
| Range       | : 0 to 600 Amp & 0 to 75 Volts |
| Least Count | : 20 Amp & 5 Volts             |

**02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION**

| SI NO. | DESCRIPTION | SR.NO.     | TRACEABILITY   | VALIDITY    | CERTIFICATE NO.  |
|--------|-------------|------------|----------------|-------------|------------------|
| 01     | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

**03 Calibration Procedure reference** AE / DFT / 02 - CM/ET/06/08

**04 Environmental Conditions** Temperature at 27.5 °C & 45 to 75 % RH

**05 Calibration Result in Volts. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 20    | 19.73             | 20             | 0.27      |
| 02     | 40    | 39.2              | 40             | 0.8       |
| 03     | 50    | 48.8              | 50             | 1.2       |
| 04     | 70    | 68.2              | 70             | 1.8       |

**Calibration Result in Amp. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 100   | 100.8             | 100            | -0.8      |
| 02     | 200   | 201.3             | 200            | -1.3      |
| 03     | 300   | 301.8             | 300            | -1.8      |
| 04     | 500   | 502               | 500            | -2        |

**06 Remarks**

01.This certificate issued as per customer requirment.

02.UUC = Unit Under Calibration.

03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.

\*\*\*\* End of Certificate \*\*\*\*

Calibrated By  
Y. P. Mute  
Calibration Engg.





Authorised By  
A. S. Choudhari  
Quality Manager

AE/RFT-50

## CALIBRATION CERTIFICATE

|                               |                                     |                                     |                                  |                       |
|-------------------------------|-------------------------------------|-------------------------------------|----------------------------------|-----------------------|
| Calibration On<br>18.Oct.2025 | Next Calibration Due<br>17.Oct.2026 | Certificate No.<br>AE/WM/25/10/1455 | Certi. Issue Date<br>24.Oct.2025 | Sheet No.<br>01 of 01 |
|-------------------------------|-------------------------------------|-------------------------------------|----------------------------------|-----------------------|

|                                                                                                 |                           |                         |          |
|-------------------------------------------------------------------------------------------------|---------------------------|-------------------------|----------|
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur. | <b>CUSTOMER REFERENCE</b> |                         |          |
|                                                                                                 | SRF No                    | : ACIPL/JC/25-26/883    |          |
|                                                                                                 | Gate Pass No.             | : -                     |          |
|                                                                                                 | Date of Receipt           | : 18.Oct.2025           |          |
| Order Inward No.                                                                                | ACIPL/25-ISO/10/883/A-140 | Location of Calibration | : Onsite |

**01 Description & Identification :**

|             |                                |
|-------------|--------------------------------|
| UUC         | : Analog Welding Machine       |
| Make        | : Panasonic                    |
| Model No.   | : YD-500KR2                    |
| Serial No.  | : D10623O0274                  |
| ID. No.     | : MIG-340                      |
| Range       | : 0 to 600 Amp & 0 to 75 Volts |
| Least Count | : 20 Amp & 5 Volts             |

**02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION**

| SI NO. | DESCRIPTION | SR.NO.     | TRACEABILITY   | VALIDITY    | CERTIFICATE NO.  |
|--------|-------------|------------|----------------|-------------|------------------|
| 01     | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

**03 Calibration Procedure reference** AE / DFT / 02 - CM/ET/06/08

**04 Environmental Conditions** Temperature at 27.5 °C & 45 to 75 % RH

**05 Calibration Result in Volts. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 20    | 20.25             | 20             | -0.25     |
| 02     | 40    | 40.4              | 40             | -0.4      |
| 03     | 50    | 50.3              | 50             | -0.3      |
| 04     | 70    | 70.8              | 70             | -0.8      |

**Calibration Result in Amp. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 100   | 99.5              | 100            | 0.5       |
| 02     | 200   | 199.2             | 200            | 0.8       |
| 03     | 300   | 299.5             | 300            | 0.5       |
| 04     | 500   | 500               | 500            | 0         |

**06 Remarks**


01.This certificate issued as per customer requirment.

02.UUC = Unit Under Calibration.

03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.

\*\*\*\* End of Certificate \*\*\*\*


  
 Calibrated By  
 Y. P. Mute  
 Calibration Engg.




  
 Authorised By  
 A. S. Choudhari  
 Quality Manager

AE/RFT-50


## CALIBRATION CERTIFICATE

|                                                                                                                                         |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
|-----------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------|-----------------------|------------------|
| Calibration On<br>18.Oct.2025                                                                                                           | Next Calibration Due<br>17.Oct.2026 | Certificate No.<br>AE/WM/25/10/1456                                                                                                                                                                                              | Certi. Issue Date<br>24.Oct.2025 | Sheet No.<br>01 of 01 |                  |
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur.                                         |                                     | CUSTOMER REFERENCE                                                                                                                                                                                                               |                                  |                       |                  |
|                                                                                                                                         |                                     | SRF No : ACIPL/JC/25-26/883                                                                                                                                                                                                      |                                  |                       |                  |
|                                                                                                                                         |                                     | Gate Pass No. : -                                                                                                                                                                                                                |                                  |                       |                  |
|                                                                                                                                         |                                     | Date of Receipt : 18.Oct.2025                                                                                                                                                                                                    |                                  |                       |                  |
| Order Inward No.                                                                                                                        | ACIPL/25-ISO/10/883/A-141           | Location of Calibration : Onsite                                                                                                                                                                                                 |                                  |                       |                  |
| 01 Description & Identification :                                                                                                       |                                     | UUC : Analog Welding Machine<br>Make : Panasonic<br>Model No. : YD-500KR2<br>Serial No. : D10623I0345<br>ID. No. : MIG-323<br>Range : 0 to 600 Amp & 0 to 75 Volts<br>Least Count : 20 Amp & 5 Volts                             |                                  |                       |                  |
| 02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION                                                                      |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| SI NO.                                                                                                                                  | DESCRIPTION                         | SR.NO.                                                                                                                                                                                                                           | TRACEBILITY                      | VALIDITY              | CERTIFICATE NO.  |
| 01                                                                                                                                      | Clamp Meter                         | 2408077674                                                                                                                                                                                                                       | NABL CC - 2632                   | 19.May.2026           | AE/CC/25-26/3349 |
| 03 Calibration Procedure reference                                                                                                      |                                     | AE / DFT / 02 - CM/ET/06/08                                                                                                                                                                                                      |                                  |                       |                  |
| 04 Environmental Conditions                                                                                                             |                                     | Temperature at 27.5 °C & 45 to 75 % RH                                                                                                                                                                                           |                                  |                       |                  |
| 05 Calibration Result in Volts. (Observed value is mean of Five reading)                                                                |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| SI No.                                                                                                                                  | Range                               | Observe on Master                                                                                                                                                                                                                | Observe on UUC                   | Deviation             |                  |
| 01                                                                                                                                      | 20                                  | 20.23                                                                                                                                                                                                                            | 20                               | -0.23                 |                  |
| 02                                                                                                                                      | 40                                  | 40.2                                                                                                                                                                                                                             | 40                               | -0.2                  |                  |
| 03                                                                                                                                      | 50                                  | 50.5                                                                                                                                                                                                                             | 50                               | -0.5                  |                  |
| 04                                                                                                                                      | 70                                  | 70.7                                                                                                                                                                                                                             | 70                               | -0.7                  |                  |
| Calibration Result in Amp. (Observed value is mean of Five reading)                                                                     |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| SI No.                                                                                                                                  | Range                               | Observe on Master                                                                                                                                                                                                                | Observe on UUC                   | Deviation             |                  |
| 01                                                                                                                                      | 100                                 | 99.8                                                                                                                                                                                                                             | 100                              | 0.2                   |                  |
| 02                                                                                                                                      | 200                                 | 199.5                                                                                                                                                                                                                            | 200                              | 0.5                   |                  |
| 03                                                                                                                                      | 300                                 | 299.5                                                                                                                                                                                                                            | 300                              | 0.5                   |                  |
| 04                                                                                                                                      | 500                                 | 500                                                                                                                                                                                                                              | 500                              | 0                     |                  |
| 06 Remarks                                                                                                                              |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| 01.This certificate issued as per customer requirment.                                                                                  |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| 02.UUC = Unit Under Calibration.                                                                                                        |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| 03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.                |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| **** End of Certificate ****                                                                                                            |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| <br>Calibrated By<br>Y. P. Mute<br>Calibration Engg. |                                     |  <br>Authorised By<br>A. S. Choudhari<br>Quality Manager |                                  |                       |                  |
| AE/RFT-50                                                                                                                               |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |

## CALIBRATION CERTIFICATE

|                                                                                                                                         |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
|-----------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------|-----------------------|------------------|
| Calibration On<br>18.Oct.2025                                                                                                           | Next Calibration Due<br>17.Oct.2026 | Certificate No.<br>AE/WM/25/10/1457                                                                                                                                                                                              | Certi. Issue Date<br>24.Oct.2025 | Sheet No.<br>01 of 01 |                  |
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur.                                         |                                     | CUSTOMER REFERENCE                                                                                                                                                                                                               |                                  |                       |                  |
|                                                                                                                                         |                                     | SRF No : ACIPL/JC/25-26/883                                                                                                                                                                                                      |                                  |                       |                  |
|                                                                                                                                         |                                     | Gate Pass No. : -                                                                                                                                                                                                                |                                  |                       |                  |
|                                                                                                                                         |                                     | Date of Receipt : 18.Oct.2025                                                                                                                                                                                                    |                                  |                       |                  |
| Order Inward No.                                                                                                                        | ACIPL/25-ISO/10/883/A-142           | Location of Calibration : Onsite                                                                                                                                                                                                 |                                  |                       |                  |
| 01 Description & Identification :                                                                                                       |                                     | UUC : Analog Welding Machine<br>Make : Panasonic<br>Model No. : YD-500KR2<br>Serial No. : D10623O0268<br>ID. No. : MIG-336<br>Range : 0 to 600 Amp & 0 to 75 Volts<br>Least Count : 20 Amp & 5 Volts                             |                                  |                       |                  |
| 02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION                                                                      |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| SI NO.                                                                                                                                  | DESCRIPTION                         | SR.NO.                                                                                                                                                                                                                           | TRACEBILITY                      | VALIDITY              | CERTIFICATE NO.  |
| 01                                                                                                                                      | Clamp Meter                         | 2408077674                                                                                                                                                                                                                       | NABL CC - 2632                   | 19.May.2026           | AE/CC/25-26/3349 |
| 03 Calibration Procedure reference                                                                                                      |                                     | AE / DFT / 02 - CM/ET/06/08                                                                                                                                                                                                      |                                  |                       |                  |
| 04 Environmental Conditions                                                                                                             |                                     | Temperature at 27.5 °C & 45 to 75 % RH                                                                                                                                                                                           |                                  |                       |                  |
| 05 Calibration Result in Volts. (Observed value is mean of Five reading)                                                                |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| SI No.                                                                                                                                  | Range                               | Observe on Master                                                                                                                                                                                                                | Observe on UUC                   | Deviation             |                  |
| 01                                                                                                                                      | 20                                  | 20.15                                                                                                                                                                                                                            | 20                               | -0.15                 |                  |
| 02                                                                                                                                      | 40                                  | 40.3                                                                                                                                                                                                                             | 40                               | -0.3                  |                  |
| 03                                                                                                                                      | 50                                  | 50.2                                                                                                                                                                                                                             | 50                               | -0.2                  |                  |
| 04                                                                                                                                      | 70                                  | 70.7                                                                                                                                                                                                                             | 70                               | -0.7                  |                  |
| Calibration Result in Amp. (Observed value is mean of Five reading)                                                                     |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| SI No.                                                                                                                                  | Range                               | Observe on Master                                                                                                                                                                                                                | Observe on UUC                   | Deviation             |                  |
| 01                                                                                                                                      | 100                                 | 100.3                                                                                                                                                                                                                            | 100                              | -0.3                  |                  |
| 02                                                                                                                                      | 200                                 | 200.8                                                                                                                                                                                                                            | 200                              | -0.8                  |                  |
| 03                                                                                                                                      | 300                                 | 300.8                                                                                                                                                                                                                            | 300                              | -0.8                  |                  |
| 04                                                                                                                                      | 500                                 | 501                                                                                                                                                                                                                              | 500                              | -1                    |                  |
| 06 Remarks                                                                                                                              |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| 01.This certificate issued as per customer requirment.                                                                                  |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| 02.UUC = Unit Under Calibration.                                                                                                        |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| 03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.                |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| **** End of Certificate ****                                                                                                            |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| <br>Calibrated By<br>Y. P. Mute<br>Calibration Engg. |                                     |  <br>Authorised By<br>A. S. Choudhari<br>Quality Manager |                                  |                       |                  |
| AE/RFT-50                                                                                                                               |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |

## CALIBRATION CERTIFICATE

|                                                                                                                                         |                                     |                                                                                                                                                                                                      |                                  |                       |
|-----------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------|-----------------------|
| Calibration On<br>18.Oct.2025                                                                                                           | Next Calibration Due<br>17.Oct.2026 | Certificate No.<br>AE/WM/25/10/1458                                                                                                                                                                  | Certi. Issue Date<br>24.Oct.2025 | Sheet No.<br>01 of 01 |
| M/s Apex Buildsys Limited.<br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur.                                                |                                     | CUSTOMER REFERENCE<br>SRF No : ACIPL/JC/25-26/883<br>Gate Pass No. : -<br>Date of Receipt : 18.Oct.2025                                                                                              |                                  |                       |
| Order Inward No.                                                                                                                        | ACIPL/25-ISO/10/883/A-143           | Location of Calibration : Onsite                                                                                                                                                                     |                                  |                       |
| 01 Description & Identification :                                                                                                       |                                     | UUC : Analog Welding Machine<br>Make : Panasonic<br>Model No. : YD-500KR2<br>Serial No. : D10623O0116<br>ID. No. : MIG-327<br>Range : 0 to 600 Amp & 0 to 75 Volts<br>Least Count : 20 Amp & 5 Volts |                                  |                       |
| 02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION                                                                      |                                     |                                                                                                                                                                                                      |                                  |                       |
| SI NO.                                                                                                                                  | DESCRIPTION                         | SR.NO.                                                                                                                                                                                               | TRACEABILITY                     | VALIDITY              |
| 01                                                                                                                                      | Clamp Meter                         | 2408077674                                                                                                                                                                                           | NABL CC - 2632                   | 19.May.2026           |
| 03 Calibration Procedure reference                                                                                                      |                                     | AE / DFT / 02 - CM/ET/06/08                                                                                                                                                                          |                                  |                       |
| 04 Environmental Conditions                                                                                                             |                                     | Temperature at 27.5 °C & 45 to 75 % RH                                                                                                                                                               |                                  |                       |
| 05 Calibration Result in Volts. (Observed value is mean of Five reading)                                                                |                                     |                                                                                                                                                                                                      |                                  |                       |
| Sl No.                                                                                                                                  | Range                               | Observe on Master                                                                                                                                                                                    | Observe on UUC                   | Deviation             |
| 01                                                                                                                                      | 20                                  | 19.74                                                                                                                                                                                                | 20                               | 0.26                  |
| 02                                                                                                                                      | 40                                  | 39.7                                                                                                                                                                                                 | 40                               | 0.3                   |
| 03                                                                                                                                      | 50                                  | 49.3                                                                                                                                                                                                 | 50                               | 0.7                   |
| 04                                                                                                                                      | 70                                  | 69.5                                                                                                                                                                                                 | 70                               | 0.5                   |
| Calibration Result in Amp. (Observed value is mean of Five reading)                                                                     |                                     |                                                                                                                                                                                                      |                                  |                       |
| Sl No.                                                                                                                                  | Range                               | Observe on Master                                                                                                                                                                                    | Observe on UUC                   | Deviation             |
| 01                                                                                                                                      | 100                                 | 99.4                                                                                                                                                                                                 | 100                              | 0.6                   |
| 02                                                                                                                                      | 200                                 | 199.2                                                                                                                                                                                                | 200                              | 0.8                   |
| 03                                                                                                                                      | 300                                 | 298.8                                                                                                                                                                                                | 300                              | 1.2                   |
| 04                                                                                                                                      | 500                                 | 498                                                                                                                                                                                                  | 500                              | 2                     |
| 06 Remarks                                                                                                                              |                                     |                                                                                                                                                                                                      |                                  |                       |
| 01.This certificate issued as per customer requirment.                                                                                  |                                     |                                                                                                                                                                                                      |                                  |                       |
| 02.UUC = Unit Under Calibration.                                                                                                        |                                     |                                                                                                                                                                                                      |                                  |                       |
| 03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.                |                                     |                                                                                                                                                                                                      |                                  |                       |
| **** End of Certificate ****                                                                                                            |                                     |                                                                                                                                                                                                      |                                  |                       |
| <br>Calibrated By<br>Y. P. Mute<br>Calibration Engg. |                                     |                               |                                  |                       |
|                                                                                                                                         |                                     | <br>Authorised By<br>A. S. Choudhari<br>Quality Manager                                                         |                                  |                       |
| AE/RFT-50                                                                                                                               |                                     |                                                                                                                                                                                                      |                                  |                       |

## CALIBRATION CERTIFICATE

|                |                      |                  |                   |           |
|----------------|----------------------|------------------|-------------------|-----------|
| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1459 | 24.Oct.2025       | 01 of 01  |

|                                                                                                 |                           |                                  |
|-------------------------------------------------------------------------------------------------|---------------------------|----------------------------------|
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur. | <b>CUSTOMER REFERENCE</b> |                                  |
|                                                                                                 | SRF No                    | : ACIPL/JC/25-26/883             |
|                                                                                                 | Gate Pass No.             | : -                              |
|                                                                                                 | Date of Receipt           | : 18.Oct.2025                    |
| Order Inward No.                                                                                | ACIPL/25-ISO/10/883/A-144 | Location of Calibration : Onsite |

**01 Description & Identification :**

|             |                                |
|-------------|--------------------------------|
| UUC         | : Analog Welding Machine       |
| Make        | : Panasonic                    |
| Model No.   | : YD-500KR2                    |
| Serial No.  | : D10623O0123                  |
| ID. No.     | : MIG-416                      |
| Range       | : 0 to 600 Amp & 0 to 75 Volts |
| Least Count | : 20 Amp & 5 Volts             |

**02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION**

| SI NO. | DESCRIPTION | SR.NO.     | TRACEBILITY    | VALIDITY    | CERTIFICATE NO.  |
|--------|-------------|------------|----------------|-------------|------------------|
| 01     | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

**03 Calibration Procedure reference** AE / DFT / 02 - CM/ET/06/08

**04 Environmental Conditions** Temperature at 27.5 °C & 45 to 75 % RH

**05 Calibration Result in Volts. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 20    | 20.15             | 20             | -0.15     |
| 02     | 40    | 40.3              | 40             | -0.3      |
| 03     | 50    | 50.2              | 50             | -0.2      |
| 04     | 70    | 70.7              | 70             | -0.7      |

**Calibration Result in Amp. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 100   | 100.3             | 100            | -0.3      |
| 02     | 200   | 200.8             | 200            | -0.8      |
| 03     | 300   | 300.8             | 300            | -0.8      |
| 04     | 500   | 501               | 500            | -1        |

**06 Remarks**


01.This certificate issued as per customer requirment.

02.UUC = Unit Under Calibration.

03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.

\*\*\*\* End of Certificate \*\*\*\*



Calibrated By  
Y. P. Mute  
Calibration Engg.





Authorised By  
A. S. Choudhari  
Quality Manager

AE/RFT-50

## CALIBRATION CERTIFICATE

|                               |                                     |                                     |                                  |                       |
|-------------------------------|-------------------------------------|-------------------------------------|----------------------------------|-----------------------|
| Calibration On<br>18.Oct.2025 | Next Calibration Due<br>17.Oct.2026 | Certificate No.<br>AE/WM/25/10/1460 | Certi. Issue Date<br>24.Oct.2025 | Sheet No.<br>01 of 01 |
|-------------------------------|-------------------------------------|-------------------------------------|----------------------------------|-----------------------|

|                                                                                                 |                           |                         |          |
|-------------------------------------------------------------------------------------------------|---------------------------|-------------------------|----------|
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur. | <b>CUSTOMER REFERENCE</b> |                         |          |
|                                                                                                 | SRF No                    | : ACIPL/JC/25-26/883    |          |
|                                                                                                 | Gate Pass No.             | : -                     |          |
|                                                                                                 | Date of Receipt           | : 18.Oct.2025           |          |
| Order Inward No.                                                                                | ACIPL/25-ISO/10/883/A-145 | Location of Calibration | : Onsite |

**01 Description & Identification :**

|             |                                |
|-------------|--------------------------------|
| UUC         | : Analog Welding Machine       |
| Make        | : Panasonic                    |
| Model No.   | : YD-500KR2                    |
| Serial No.  | : D10623O0223                  |
| ID. No.     | : MIG-417                      |
| Range       | : 0 to 600 Amp & 0 to 75 Volts |
| Least Count | : 20 Amp & 5 Volts             |

**02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION**

| SI NO. | DESCRIPTION | SR.NO.     | TRACEBILITY    | VALIDITY    | CERTIFICATE NO.  |
|--------|-------------|------------|----------------|-------------|------------------|
| 01     | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

**03 Calibration Procedure reference** AE / DFT / 02 - CM/ET/06/08

**04 Environmental Conditions** Temperature at 27.5 °C & 45 to 75 % RH

**05 Calibration Result in Volts. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 20    | 20.32             | 20             | -0.32     |
| 02     | 40    | 40.5              | 40             | -0.5      |
| 03     | 50    | 50.8              | 50             | -0.8      |
| 04     | 70    | 70.8              | 70             | -0.8      |

**Calibration Result in Amp. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 100   | 100.5             | 100            | -0.5      |
| 02     | 200   | 200.5             | 200            | -0.5      |
| 03     | 300   | 300.8             | 300            | -0.8      |
| 04     | 500   | 501               | 500            | -1        |

**06 Remarks**


01.This certificate issued as per customer requirment.

02.UUC = Unit Under Calibration.

03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.

\*\*\*\* End of Certificate \*\*\*\*

  
 Calibrated By  
 Y. P. Mute  
 Calibration Engg.

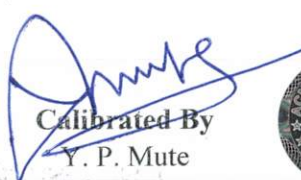

  
 Authorised By  
 A. S. Choudhari  
 Quality Manager

AE/RFT-50

## CALIBRATION CERTIFICATE

|                |                      |                  |                   |           |
|----------------|----------------------|------------------|-------------------|-----------|
| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1461 | 24.Oct.2025       | 01 of 01  |

|                                                                                                 |                           |                      |
|-------------------------------------------------------------------------------------------------|---------------------------|----------------------|
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur. | <b>CUSTOMER REFERENCE</b> |                      |
|                                                                                                 | SRF No                    | : ACIPL/JC/25-26/883 |
|                                                                                                 | Gate Pass No.             | : -                  |
|                                                                                                 | Date of Receipt           | : 18.Oct.2025        |

|                  |                           |                         |          |
|------------------|---------------------------|-------------------------|----------|
| Order Inward No. | ACIPL/25-ISO/10/883/A-146 | Location of Calibration | : Onsite |
|------------------|---------------------------|-------------------------|----------|

**01 Description & Identification** :

|             |                                |
|-------------|--------------------------------|
| UUC         | : Analog Welding Machine       |
| Make        | : Panasonic                    |
| Model No.   | : YD-500KR2                    |
| Serial No.  | : D10623G0218                  |
| ID. No.     | : MIG-345                      |
| Range       | : 0 to 600 Amp & 0 to 75 Volts |
| Least Count | : 20 Amp & 5 Volts             |

**02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION**

| SI NO. | DESCRIPTION | SR.NO.     | TRACEBILITY    | VALIDITY    | CERTIFICATE NO.  |
|--------|-------------|------------|----------------|-------------|------------------|
| 01     | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

**03 Calibration Procedure reference** AE / DFT / 02 - CM/ET/06/08

**04 Environmental Conditions** Temperature at 27.5 °C & 45 to 75 % RH

**05 Calibration Result in Volts. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 20    | 20.25             | 20             | -0.25     |
| 02     | 40    | 40.3              | 40             | -0.3      |
| 03     | 50    | 50.8              | 50             | -0.8      |
| 04     | 70    | 70.8              | 70             | -0.8      |

**Calibration Result in Amp. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 100   | 100.5             | 100            | -0.5      |
| 02     | 200   | 200.5             | 200            | -0.5      |
| 03     | 300   | 300.8             | 300            | -0.8      |
| 04     | 500   | 501               | 500            | -1        |

**06 Remarks**


01.This certificate issued as per customer requirment.

02.UUC = Unit Under Calibration.

03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.

\*\*\*\* End of Certificate \*\*\*\*

  
 Calibrated By  
 Y. P. Mute  
 Calibration Engg.



  
 Authorised By  
 A. S. Choudhari  
 Quality Manager

AE/RFT-50

## CALIBRATION CERTIFICATE

|                |                      |                  |                   |           |
|----------------|----------------------|------------------|-------------------|-----------|
| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1462 | 24.Oct.2025       | 01 of 01  |

|                                                                                                 |                           |                      |
|-------------------------------------------------------------------------------------------------|---------------------------|----------------------|
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur. | <b>CUSTOMER REFERENCE</b> |                      |
|                                                                                                 | SRF No                    | : ACIPL/JC/25-26/883 |
|                                                                                                 | Gate Pass No.             | : -                  |
|                                                                                                 | Date of Receipt           | : 18.Oct.2025        |

|                  |                           |                         |          |
|------------------|---------------------------|-------------------------|----------|
| Order Inward No. | ACIPL/25-ISO/10/883/A-147 | Location of Calibration | : Onsite |
|------------------|---------------------------|-------------------------|----------|

|                                 |             |                                |
|---------------------------------|-------------|--------------------------------|
| 01 Description & Identification | : UUC       | : Digital Mig Welding Machine  |
|                                 | Make        | : PANASONIC                    |
|                                 | Model No.   | : KRII-500                     |
|                                 | Serial No.  | : -                            |
|                                 | ID. No.     | : PANA-009                     |
|                                 | Range       | : 0 to 400 Amp & 0 to 75 Volts |
|                                 | Least Count | : 20 Amp & 2 Volts             |

| 02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION |             |            |                |             |                  |
|--------------------------------------------------------------------|-------------|------------|----------------|-------------|------------------|
| SI NO.                                                             | DESCRIPTION | SR.NO.     | TRACEABILITY   | VALIDITY    | CERTIFICATE NO.  |
| 01                                                                 | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

|                                    |                             |
|------------------------------------|-----------------------------|
| 03 Calibration Procedure reference | AE / DFT / 02 - CM/ET/06/08 |
|------------------------------------|-----------------------------|

|                             |                                        |
|-----------------------------|----------------------------------------|
| 04 Environmental Conditions | Temperature at 27.5 °C & 45 to 75 % RH |
|-----------------------------|----------------------------------------|

| 05 Calibration Result in Volts. (Observed value is mean of Five reading) |       |                   |                |           |
|--------------------------------------------------------------------------|-------|-------------------|----------------|-----------|
| SI No.                                                                   | Range | Observe on Master | Observe on UUC | Deviation |
| 01                                                                       | 20    | 20.25             | 20             | -0.25     |
| 02                                                                       | 50    | 50.5              | 50             | -0.5      |
| 03                                                                       | 70    | 70.8              | 70             | -0.8      |

| Calibration Result in Amp. (Observed value is mean of Five reading) |       |                   |                |           |
|---------------------------------------------------------------------|-------|-------------------|----------------|-----------|
| SI No.                                                              | Range | Observe on Master | Observe on UUC | Deviation |
| 01                                                                  | 50    | 50.4              | 50             | -0.4      |
| 02                                                                  | 100   | 100.8             | 100            | -0.8      |
| 03                                                                  | 200   | 201.2             | 200            | -1.2      |
| 04                                                                  | 300   | 301               | 300            | -1        |


  

|                                                                                                                          |  |
|--------------------------------------------------------------------------------------------------------------------------|--|
| 06 Remarks                                                                                                               |  |
| 01.This certificate issued as per customer requirment.                                                                   |  |
| 02.UUC = Unit Under Calibration.                                                                                         |  |
| 03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories. |  |

\*\*\*\* End of Certificate \*\*\*\*

  
 Calibrated By  
 Y. P. Mute  
 Calibration Engg.



  
 Authorised By  
 A. S. Choudhari  
 Quality Manager

AE/RFT-50

## CALIBRATION CERTIFICATE

|                |                      |                  |                   |           |
|----------------|----------------------|------------------|-------------------|-----------|
| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1463 | 24.Oct.2025       | 01 of 01  |

|                                                                                                 |                           |                      |
|-------------------------------------------------------------------------------------------------|---------------------------|----------------------|
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur. | <b>CUSTOMER REFERENCE</b> |                      |
|                                                                                                 | SRF No                    | : ACIPL/JC/25-26/883 |
|                                                                                                 | Gate Pass No.             | : -                  |
|                                                                                                 | Date of Receipt           | : 18.Oct.2025        |

|                  |                           |                         |          |
|------------------|---------------------------|-------------------------|----------|
| Order Inward No. | ACIPL/25-ISO/10/883/A-148 | Location of Calibration | : Onsite |
|------------------|---------------------------|-------------------------|----------|

|                                 |             |                                |
|---------------------------------|-------------|--------------------------------|
| 01 Description & Identification | UUC         | : Analog Welding Machine       |
|                                 | Make        | : Panasonic                    |
|                                 | Model No.   | : YD-500KR2                    |
|                                 | Serial No.  | : D10623O0209                  |
|                                 | ID. No.     | : MIG-337                      |
|                                 | Range       | : 0 to 600 Amp & 0 to 75 Volts |
|                                 | Least Count | : 20 Amp & 5 Volts             |

| 02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION |             |            |                |             |                  |
|--------------------------------------------------------------------|-------------|------------|----------------|-------------|------------------|
| SI NO.                                                             | DESCRIPTION | SR.NO.     | TRACEABILITY   | VALIDITY    | CERTIFICATE NO.  |
| 01                                                                 | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

|                                    |                             |
|------------------------------------|-----------------------------|
| 03 Calibration Procedure reference | AE / DFT / 02 - CM/ET/06/08 |
|------------------------------------|-----------------------------|

|                             |                                        |
|-----------------------------|----------------------------------------|
| 04 Environmental Conditions | Temperature at 27.5 °C & 45 to 75 % RH |
|-----------------------------|----------------------------------------|

| 05 Calibration Result in Volts. (Observed value is mean of Five reading) |       |                   |                |           |
|--------------------------------------------------------------------------|-------|-------------------|----------------|-----------|
| SI No.                                                                   | Range | Observe on Master | Observe on UUC | Deviation |
| 01                                                                       | 20    | 20.22             | 20             | -0.22     |
| 02                                                                       | 40    | 40.5              | 40             | -0.5      |
| 03                                                                       | 50    | 50.3              | 50             | -0.3      |
| 04                                                                       | 70    | 70.8              | 70             | -0.8      |


  

| Calibration Result in Amp. (Observed value is mean of Five reading) |       |                   |                |           |
|---------------------------------------------------------------------|-------|-------------------|----------------|-----------|
| SI No.                                                              | Range | Observe on Master | Observe on UUC | Deviation |
| 01                                                                  | 100   | 99.7              | 100            | 0.3       |
| 02                                                                  | 200   | 199.2             | 200            | 0.8       |
| 03                                                                  | 300   | 299.1             | 300            | 0.9       |
| 04                                                                  | 500   | 499               | 500            | 1         |

|                                                                                                                          |  |
|--------------------------------------------------------------------------------------------------------------------------|--|
| 06 Remarks                                                                                                               |  |
| 01.This certificate issued as per customer requirment.                                                                   |  |
| 02.UUC = Unit Under Calibration.                                                                                         |  |
| 03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories. |  |
| **** End of Certificate ****                                                                                             |  |

  
 Calibrated By  
 Y. P. Mute  
 Calibration Engg.

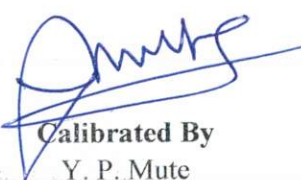

  
 Authorised By  
 A. S. Choudhari  
 Quality Manager

AE/RFT-50

## CALIBRATION CERTIFICATE

|                |                      |                  |                   |           |
|----------------|----------------------|------------------|-------------------|-----------|
| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1464 | 24.Oct.2025       | 01 of 01  |

|                                                                                                 |                           |                      |
|-------------------------------------------------------------------------------------------------|---------------------------|----------------------|
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur. | <b>CUSTOMER REFERENCE</b> |                      |
|                                                                                                 | SRF No                    | : ACIPL/JC/25-26/883 |
|                                                                                                 | Gate Pass No.             | : -                  |
|                                                                                                 | Date of Receipt           | : 18.Oct.2025        |

|                  |                           |                         |          |
|------------------|---------------------------|-------------------------|----------|
| Order Inward No. | ACIPL/25-ISO/10/883/A-149 | Location of Calibration | : Onsite |
|------------------|---------------------------|-------------------------|----------|

|                                 |             |                                |
|---------------------------------|-------------|--------------------------------|
| 01 Description & Identification | UUC         | : Analog Welding Machine       |
|                                 | Make        | : Panasonic                    |
|                                 | Model No.   | : YD-500KR2                    |
|                                 | Serial No.  | : D10623N0003                  |
|                                 | ID. No.     | : MIG-301                      |
|                                 | Range       | : 0 to 600 Amp & 0 to 75 Volts |
|                                 | Least Count | : 20 Amp & 5 Volts             |

| 02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION |             |            |                |             |                  |
|--------------------------------------------------------------------|-------------|------------|----------------|-------------|------------------|
| SI NO.                                                             | DESCRIPTION | SR.NO.     | TRACEABILITY   | VALIDITY    | CERTIFICATE NO.  |
| 01                                                                 | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

|                                    |                             |
|------------------------------------|-----------------------------|
| 03 Calibration Procedure reference | AE / DFT / 02 - CM/ET/06/08 |
|------------------------------------|-----------------------------|

|                             |                                        |
|-----------------------------|----------------------------------------|
| 04 Environmental Conditions | Temperature at 27.5 °C & 45 to 75 % RH |
|-----------------------------|----------------------------------------|

| 05 Calibration Result in Volts. (Observed value is mean of Five reading) |       |                   |                |           |
|--------------------------------------------------------------------------|-------|-------------------|----------------|-----------|
| Sl No.                                                                   | Range | Observe on Master | Observe on UUC | Deviation |
| 01                                                                       | 20    | 20.43             | 20             | -0.43     |
| 02                                                                       | 40    | 40.8              | 40             | -0.8      |
| 03                                                                       | 50    | 51.3              | 50             | -1.3      |
| 04                                                                       | 70    | 71.8              | 70             | -1.8      |


  

| Calibration Result in Amp. (Observed value is mean of Five reading) |       |                   |                |           |
|---------------------------------------------------------------------|-------|-------------------|----------------|-----------|
| Sl No.                                                              | Range | Observe on Master | Observe on UUC | Deviation |
| 01                                                                  | 100   | 100.7             | 100            | -0.7      |
| 02                                                                  | 200   | 201.2             | 200            | -1.2      |
| 03                                                                  | 300   | 301.5             | 300            | -1.5      |
| 04                                                                  | 500   | 502               | 500            | -2        |

|                                                                                                                          |  |
|--------------------------------------------------------------------------------------------------------------------------|--|
| 06 Remarks                                                                                                               |  |
| 01.This certificate issued as per customer requirment.                                                                   |  |
| 02.UUC = Unit Under Calibration.                                                                                         |  |
| 03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories. |  |
| **** End of Certificate ****                                                                                             |  |

  
 Calibrated By  
 Y. P. Mute  
 Calibration Engg.



  
 Authorised By  
 A. S. Choudhari  
 Quality Manager

AE/RFT-50

## CALIBRATION CERTIFICATE

|                |                      |                  |                   |           |
|----------------|----------------------|------------------|-------------------|-----------|
| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1465 | 24.Oct.2025       | 01 of 01  |

|                                                                                          |                    |                      |
|------------------------------------------------------------------------------------------|--------------------|----------------------|
| M/s Apex Buildsys Limited.<br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur. | CUSTOMER REFERENCE |                      |
|                                                                                          | SRF No             | : ACIPL/JC/25-26/883 |
|                                                                                          | Gate Pass No.      | : -                  |
|                                                                                          | Date of Receipt    | : 18.Oct.2025        |

|                  |                           |                         |          |
|------------------|---------------------------|-------------------------|----------|
| Order Inward No. | ACIPL/25-ISO/10/883/A-150 | Location of Calibration | : Onsite |
|------------------|---------------------------|-------------------------|----------|

|                                 |   |             |                                |
|---------------------------------|---|-------------|--------------------------------|
| 01 Description & Identification | : | UUC         | : Analog Welding Machine       |
|                                 |   | Make        | : Panasonic                    |
|                                 |   | Model No.   | : YD-500KR2                    |
|                                 |   | Serial No.  | : D10623O0073                  |
|                                 |   | ID. No.     | : MIG-422                      |
|                                 |   | Range       | : 0 to 600 Amp & 0 to 75 Volts |
|                                 |   | Least Count | : 20 Amp & 5 Volts             |

|                                                                    |             |            |                |             |                  |
|--------------------------------------------------------------------|-------------|------------|----------------|-------------|------------------|
| 02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION |             |            |                |             |                  |
| SI NO.                                                             | DESCRIPTION | SR.NO.     | TRACEBILITY    | VALIDITY    | CERTIFICATE NO.  |
| 01                                                                 | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

|                                    |                             |
|------------------------------------|-----------------------------|
| 03 Calibration Procedure reference | AE / DFT / 02 - CM/ET/06/08 |
|------------------------------------|-----------------------------|

|                             |                                        |
|-----------------------------|----------------------------------------|
| 04 Environmental Conditions | Temperature at 27.5 °C & 45 to 75 % RH |
|-----------------------------|----------------------------------------|

|                                                                          |       |                   |                |           |
|--------------------------------------------------------------------------|-------|-------------------|----------------|-----------|
| 05 Calibration Result in Volts. (Observed value is mean of Five reading) |       |                   |                |           |
| SI No.                                                                   | Range | Observe on Master | Observe on UUC | Deviation |
| 01                                                                       | 20    | 20.28             | 20             | -0.28     |
| 02                                                                       | 40    | 40.2              | 40             | -0.2      |
| 03                                                                       | 50    | 50.5              | 50             | -0.5      |
| 04                                                                       | 70    | 70.8              | 70             | -0.8      |


  

|                                                                     |       |                   |                |           |
|---------------------------------------------------------------------|-------|-------------------|----------------|-----------|
| Calibration Result in Amp. (Observed value is mean of Five reading) |       |                   |                |           |
| SI No.                                                              | Range | Observe on Master | Observe on UUC | Deviation |
| 01                                                                  | 100   | 101.2             | 100            | -1.2      |
| 02                                                                  | 200   | 201.8             | 200            | -1.8      |
| 03                                                                  | 300   | 301.5             | 300            | -1.5      |
| 04                                                                  | 500   | 502               | 500            | -2        |

|                                                                                                                          |  |
|--------------------------------------------------------------------------------------------------------------------------|--|
| 06 Remarks                                                                                                               |  |
| 01.This certificate issued as per customer requirment.                                                                   |  |
| 02.UUC = Unit Under Calibration.                                                                                         |  |
| 03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories. |  |
| **** End of Certificate ****                                                                                             |  |

|                                                                                                                                         |                                                                                     |                                                                                      |                                                                                                                                              |
|-----------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------|
| <br>Calibrated By<br>Y. P. Mute<br>Calibration Engg. |  |  | <br>Authorised By<br>A. S. Choudhari<br>Quality Manager |
|-----------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------|

AE/RFT-50
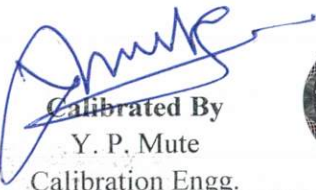
## CALIBRATION CERTIFICATE

|                |                      |                  |                   |           |
|----------------|----------------------|------------------|-------------------|-----------|
| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1466 | 24.Oct.2025       | 01 of 01  |

|                                                                                                 |                           |                         |          |
|-------------------------------------------------------------------------------------------------|---------------------------|-------------------------|----------|
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur. | <b>CUSTOMER REFERENCE</b> |                         |          |
|                                                                                                 | SRF No                    | : ACIPL/JC/25-26/883    |          |
|                                                                                                 | Gate Pass No.             | : -                     |          |
|                                                                                                 | Date of Receipt           | : 18.Oct.2025           |          |
| Order Inward No.                                                                                | ACIPL/25-ISO/10/883/A-151 | Location of Calibration | : Onsite |

**01 Description & Identification** :

|             |                                |
|-------------|--------------------------------|
| UUC         | : Analog Welding Machine       |
| Make        | : Panasonic                    |
| Model No.   | : YD-500KR2                    |
| Serial No.  | : D10623I0343                  |
| ID. No.     | : MIG-330                      |
| Range       | : 0 to 600 Amp & 0 to 75 Volts |
| Least Count | : 20 Amp & 5 Volts             |

**02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION**

| SI NO. | DESCRIPTION | SR.NO.     | TRACEABILITY   | VALIDITY    | CERTIFICATE NO.  |
|--------|-------------|------------|----------------|-------------|------------------|
| 01     | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

**03 Calibration Procedure reference** AE / DFT / 02 - CM/ET/06/08

**04 Environmental Conditions** Temperature at 27.5 °C & 45 to 75 % RH

**05 Calibration Result in Volts. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 20    | 19.85             | 20             | 0.15      |
| 02     | 40    | 39.7              | 40             | 0.3       |
| 03     | 50    | 49.5              | 50             | 0.5       |
| 04     | 70    | 68.8              | 70             | 1.2       |

**Calibration Result in Amp. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 100   | 99.8              | 100            | 0.2       |
| 02     | 200   | 199.5             | 200            | 0.5       |
| 03     | 300   | 298.3             | 300            | 1.7       |
| 04     | 500   | 498               | 500            | 2         |

**06 Remarks**


01.This certificate issued as per customer requirment.

02.UUC = Unit Under Calibration.

03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.

\*\*\*\* End of Certificate \*\*\*\*



Calibrated By  
Y. P. Mute  
Calibration Engg.







Authorised By  
A. S. Choudhari  
Quality Manager

AE/RFT-50

## CALIBRATION CERTIFICATE

|                |                      |                  |                   |           |
|----------------|----------------------|------------------|-------------------|-----------|
| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1467 | 24.Oct.2025       | 01 of 01  |

|                                                                                                 |                           |                         |          |
|-------------------------------------------------------------------------------------------------|---------------------------|-------------------------|----------|
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur. | <b>CUSTOMER REFERENCE</b> |                         |          |
|                                                                                                 | SRF No                    | : ACIPL/JC/25-26/883    |          |
|                                                                                                 | Gate Pass No.             | : -                     |          |
|                                                                                                 | Date of Receipt           | : 18.Oct.2025           |          |
| Order Inward No.                                                                                | ACIPL/25-ISO/10/883/A-152 | Location of Calibration | : Onsite |

**01 Description & Identification :**

|             |                               |
|-------------|-------------------------------|
| UUC         | : Digital Arc Welding Machine |
| Make        | : Ador                        |
| Model No.   | : CHAMP-600                   |
| Serial No.  | : 79/24073770                 |
| ID. No.     | : MEC-226                     |
| Range       | : 0 to 600 Amp & 0 to 44 Volt |
| Least Count | : 1 Amp & 0.1 Volt            |

**02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION**

| SI NO. | DESCRIPTION | SR.NO.     | TRACEABILITY   | VALIDITY    | CERTIFICATE NO.  |
|--------|-------------|------------|----------------|-------------|------------------|
| 01     | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

**03 Calibration Procedure reference** AE / DFT / 02 - CM/ET/06/08

**04 Environmental Conditions** Temperature at 27.5 °C & 45 to 75 % RH

**05 Calibration Result in Volts. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 20    | 20.25             | 20.5           | 0.25      |
| 02     | 30    | 30.21             | 31.3           | 1.09      |
| 03     | 40    | 39.7              | 41.5           | 1.8       |

**Calibration Result in Amp. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 200   | 200.8             | 200            | -0.8      |
| 02     | 400   | 400               | 400            | 0         |
| 03     | 500   | 500               | 501            | 1         |
| 04     | 600   | 600               | 601            | 1         |

**Remarks**

01.This certificate issued as per customer requirment.


02.UUC = Unit Under Calibration.

03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.

\*\*\*\* End of Certificate \*\*\*\*

**Calibrated By**  
Y. P. Mute  
Calibration Engg.






**Authorised By**  
A. S. Choudhari  
Quality Manager



AE/RFT-50

## CALIBRATION CERTIFICATE

|                |                      |                  |                   |           |
|----------------|----------------------|------------------|-------------------|-----------|
| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1468 | 24.Oct.2025       | 01 of 01  |

|                                                                                                 |                           |                      |
|-------------------------------------------------------------------------------------------------|---------------------------|----------------------|
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur. | <b>CUSTOMER REFERENCE</b> |                      |
|                                                                                                 | SRF No                    | : ACIPL/JC/25-26/883 |
|                                                                                                 | Gate Pass No.             | : -                  |
|                                                                                                 | Date of Receipt           | : 18.Oct.2025        |

|                  |                           |                         |          |
|------------------|---------------------------|-------------------------|----------|
| Order Inward No. | ACIPL/25-ISO/10/883/A-153 | Location of Calibration | : Onsite |
|------------------|---------------------------|-------------------------|----------|

**01 Description & Identification**

|             |                               |
|-------------|-------------------------------|
| UUC         | : Digital Arc Welding Machine |
| Make        | : Ador                        |
| Model No.   | : CHAMP-600                   |
| Serial No.  | : 79/23094819                 |
| ID. No.     | : MEC-209                     |
| Range       | : 0 to 600 Amp & 0 to 44 Volt |
| Least Count | : 1 Amp & 0.1 Volt            |

**02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION**

| SI NO. | DESCRIPTION | SR.NO.     | TRACEBILITY    | VALIDITY    | CERTIFICATE NO.  |
|--------|-------------|------------|----------------|-------------|------------------|
| 01     | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

**03 Calibration Procedure reference** AE / DFT / 02 - CM/ET/06/08

**04 Environmental Conditions** Temperature at 27.5 °C & 45 to 75 % RH

**05 Calibration Result in Volts. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 20    | 20.38             | 20.5           | 0.12      |
| 02     | 30    | 30.52             | 30.8           | 0.28      |
| 03     | 40    | 40.8              | 41.5           | 0.7       |

**Calibration Result in Amp. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 200   | 200.5             | 200            | -0.5      |
| 02     | 400   | 400               | 401            | 1         |
| 03     | 500   | 499               | 501            | 2         |
| 04     | 600   | 600               | 602            | 2         |

**Remarks**


01.This certificate issued as per customer requirment.

02.UUC = Unit Under Calibration.

03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.

\*\*\*\* End of Certificate \*\*\*\*

  
 Calibrated By  
 Y. P. Mute  
 Calibration Engg.



  
 Authorised By  
 A. S. Choudhari  
 Quality Manager

AE/RFT-50

## CALIBRATION CERTIFICATE

|                |                      |                  |                   |           |
|----------------|----------------------|------------------|-------------------|-----------|
| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1469 | 24.Oct.2025       | 01 of 01  |

|                                                                                                 |                           |                      |
|-------------------------------------------------------------------------------------------------|---------------------------|----------------------|
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur. | <b>CUSTOMER REFERENCE</b> |                      |
|                                                                                                 | SRF No                    | : ACIPL/JC/25-26/883 |
|                                                                                                 | Gate Pass No.             | : -                  |
|                                                                                                 | Date of Receipt           | : 18.Oct.2025        |

|                  |                           |                         |          |
|------------------|---------------------------|-------------------------|----------|
| Order Inward No. | ACIPL/25-ISO/10/883/A-154 | Location of Calibration | : Onsite |
|------------------|---------------------------|-------------------------|----------|

**01 Description & Identification :**

|             |                               |
|-------------|-------------------------------|
| UUC         | : Digital Arc Welding Machine |
| Make        | : Ador                        |
| Model No.   | : CHAMP-600                   |
| Serial No.  | : 79/23116615                 |
| ID. No.     | : MEC-234                     |
| Range       | : 0 to 600 Amp & 0 to 44 Volt |
| Least Count | : 1 Amp & 0.1 Volt            |

**02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION**

| SI NO. | DESCRIPTION | SR.NO.     | TRACEABILITY   | VALIDITY    | CERTIFICATE NO.  |
|--------|-------------|------------|----------------|-------------|------------------|
| 01     | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

**03 Calibration Procedure reference** AE / DFT / 02 - CM/ET/06/08

**04 Environmental Conditions** Temperature at 27.5 °C & 45 to 75 % RH

**05 Calibration Result in Volts. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 20    | 20.12             | 20.3           | 0.18      |
| 02     | 30    | 30.43             | 30.8           | 0.37      |
| 03     | 40    | 40.5              | 40.8           | 0.3       |

**Calibration Result in Amp. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 200   | 200.3             | 200            | -0.3      |
| 02     | 400   | 400               | 401            | 1         |
| 03     | 500   | 499               | 501            | 2         |
| 04     | 600   | 600               | 601            | 1         |

**Remarks**


01.This certificate issued as per customer requirment.

02.UUC = Unit Under Calibration.

03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.

\*\*\*\* End of Certificate \*\*\*\*

  
 Calibrated By  
 Y. P. Mute  
 Calibration Engg.

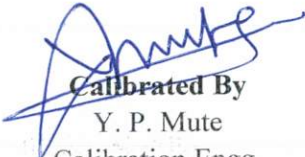

  
 Authorised By  
 A. S. Choudhari  
 Quality Manager

AE/RFT-50

## CALIBRATION CERTIFICATE

|                |                      |                  |                   |           |
|----------------|----------------------|------------------|-------------------|-----------|
| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1470 | 24.Oct.2025       | 01 of 01  |

|                                                                                                 |                           |                      |
|-------------------------------------------------------------------------------------------------|---------------------------|----------------------|
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur. | <b>CUSTOMER REFERENCE</b> |                      |
|                                                                                                 | SRF No                    | : ACIPL/JC/25-26/883 |
|                                                                                                 | Gate Pass No.             | : -                  |
|                                                                                                 | Date of Receipt           | : 18.Oct.2025        |

|                  |                           |                         |          |
|------------------|---------------------------|-------------------------|----------|
| Order Inward No. | ACIPL/25-ISO/10/883/A-155 | Location of Calibration | : Onsite |
|------------------|---------------------------|-------------------------|----------|

**01 Description & Identification**

|             |                               |
|-------------|-------------------------------|
| UUC         | : Digital Arc Welding Machine |
| Make        | : Ador                        |
| Model No.   | : CHAMP-600                   |
| Serial No.  | : 79/23116710                 |
| ID. No.     | : MEC-236                     |
| Range       | : 0 to 600 Amp & 0 to 44 Volt |
| Least Count | : 1 Amp & 0.1 Volt            |

**02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION**

| SI NO. | DESCRIPTION | SR.NO.     | TRACEABILITY   | VALIDITY    | CERTIFICATE NO.  |
|--------|-------------|------------|----------------|-------------|------------------|
| 01     | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

**03 Calibration Procedure reference** AE / DFT / 02 - CM/ET/06/08

**04 Environmental Conditions** Temperature at 27.5 °C & 45 to 75 % RH

**05 Calibration Result in Volts. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 20    | 20.25             | 20.7           | 0.45      |
| 02     | 30    | 30.2              | 31.2           | 0.97      |
| 03     | 40    | 40.3              | 41.5           | 1.2       |

**Calibration Result in Amp. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 200   | 200.3             | 200            | -0.3      |
| 02     | 400   | 400               | 400            | 0         |
| 03     | 500   | 500               | 500            | 0         |
| 04     | 600   | 600               | 601            | 1         |

**06 Remarks**


01.This certificate issued as per customer requirment.

02.UUC = Unit Under Calibration.

03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.

\*\*\*\* End of Certificate \*\*\*\*

  
 Calibrated By  
 Y. P. Mute  
 Calibration Engg.



  
 Authorised By  
 A. S. Choudhari  
 Quality Manager

AE/RFT-50

## CALIBRATION CERTIFICATE

|                |                      |                  |                   |           |
|----------------|----------------------|------------------|-------------------|-----------|
| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1471 | 24.Oct.2025       | 01 of 01  |

|                                                                                                 |                           |                      |
|-------------------------------------------------------------------------------------------------|---------------------------|----------------------|
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur. | <b>CUSTOMER REFERENCE</b> |                      |
|                                                                                                 | SRF No                    | : ACIPL/JC/25-26/883 |
|                                                                                                 | Gate Pass No.             | : -                  |
|                                                                                                 | Date of Receipt           | : 18.Oct.2025        |

|                  |                           |                         |          |
|------------------|---------------------------|-------------------------|----------|
| Order Inward No. | ACIPL/25-ISO/10/883/A-156 | Location of Calibration | : Onsite |
|------------------|---------------------------|-------------------------|----------|

**01 Description & Identification**

|             |                                |
|-------------|--------------------------------|
| UUC         | : Mig Welding Machine          |
| Make        | : Panasonic                    |
| Model No.   | : YD-630AT3                    |
| Serial No.  | : D31125T0012                  |
| ID. No.     | : MIG-418                      |
| Range       | : 0 to 600 Amp & 0 to 75 Volts |
| Least Count | : 20 Amp & 5 Volts             |

**02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION**

| SI NO. | DESCRIPTION | SR.NO.     | TRACEBILITY    | VALIDITY    | CERTIFICATE NO.  |
|--------|-------------|------------|----------------|-------------|------------------|
| 01     | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

**03 Calibration Procedure reference** AE / DFT / 02 - CM/ET/06/08

**04 Environmental Conditions** Temperature at 27.5 °C & 45 to 75 % RH

**05 Calibration Result in Volts. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 20    | 20.23             | 20             | -0.23     |
| 02     | 40    | 40.3              | 40             | -0.3      |
| 03     | 50    | 50.5              | 50             | -0.5      |
| 04     | 70    | 70.8              | 70             | -0.8      |

**Calibration Result in Amp. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 100   | 100.3             | 100            | -0.3      |
| 02     | 200   | 200.8             | 200            | -0.8      |
| 03     | 300   | 300.5             | 300            | -0.5      |
| 04     | 500   | 500               | 500            | 0         |

**06 Remarks**


01.This certificate issued as per customer requirement.

02.UUC = Unit Under Calibration.

03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.

\*\*\*\* End of Certificate \*\*\*\*

  
 Calibrated By  
 Y. P. Mute  
 Calibration Engg.



  
 Authorised By  
 A. S. Choudhari  
 Quality Manager

AE/RFT-50

## CALIBRATION CERTIFICATE

|                |                      |                  |                   |           |
|----------------|----------------------|------------------|-------------------|-----------|
| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1472 | 24.Oct.2025       | 01 of 01  |

|                                                                                                 |                           |                         |          |
|-------------------------------------------------------------------------------------------------|---------------------------|-------------------------|----------|
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur. | <b>CUSTOMER REFERENCE</b> |                         |          |
|                                                                                                 | SRF No                    | : ACIPL/JC/25-26/883    |          |
|                                                                                                 | Gate Pass No.             | : -                     |          |
|                                                                                                 | Date of Receipt           | : 18.Oct.2025           |          |
| Order Inward No.                                                                                | ACIPL/25-ISO/10/883/A-157 | Location of Calibration | : Onsite |

|                                 |             |                               |
|---------------------------------|-------------|-------------------------------|
| 01 Description & Identification | : UUC       | : Digital Arc Welding Machine |
|                                 | Make        | : Ador                        |
|                                 | Model No.   | : CHAMP-600                   |
|                                 | Serial No.  | : 79/23116614                 |
|                                 | ID. No.     | : MEC-237                     |
|                                 | Range       | : 0 to 600 Amp & 0 to 44 Volt |
|                                 | Least Count | : 1 Amp & 0.1 Volt            |

| 02 MASTER EQUIPMENTS AND TRACEABILITY DETAILS USED FOR CALIBRATION |             |            |                |             |                  |
|--------------------------------------------------------------------|-------------|------------|----------------|-------------|------------------|
| SI NO.                                                             | DESCRIPTION | SR.NO.     | TRACEBILITY    | VALIDITY    | CERTIFICATE NO.  |
| 01                                                                 | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

| 03 Calibration Procedure reference                                       | AE / DFT / 02 - CM/ET/06/08            |                   |                |           |
|--------------------------------------------------------------------------|----------------------------------------|-------------------|----------------|-----------|
| 04 Environmental Conditions                                              | Temperature at 27.5 °C & 45 to 75 % RH |                   |                |           |
| 05 Calibration Result in Volts. (Observed value is mean of Five reading) |                                        |                   |                |           |
| SI No.                                                                   | Range                                  | Observe on Master | Observe on UUC | Deviation |
| 01                                                                       | 20                                     | 20.25             | 20.7           | 0.45      |
| 02                                                                       | 30                                     | 30.48             | 31.3           | 0.82      |
| 03                                                                       | 40                                     | 40.3              | 41.8           | 1.5       |


  

| Calibration Result in Amp. (Observed value is mean of Five reading) |       |                   |                |           |
|---------------------------------------------------------------------|-------|-------------------|----------------|-----------|
| SI No.                                                              | Range | Observe on Master | Observe on UUC | Deviation |
| 01                                                                  | 200   | 200.5             | 200            | -0.5      |
| 02                                                                  | 400   | 400               | 400            | 0         |
| 03                                                                  | 500   | 500               | 500            | 0         |
| 04                                                                  | 600   | 600               | 600            | 0         |

|                                                                                                                          |
|--------------------------------------------------------------------------------------------------------------------------|
| 06 Remarks                                                                                                               |
| 01.This certificate issued as per customer requirment.                                                                   |
| 02.UUC = Unit Under Calibration.                                                                                         |
| 03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories. |
| **** End of Certificate ****                                                                                             |



  
 Calibrated By  
 Y. P. Mute  
 Calibration Engg.



  
 Authorised By  
 A. S. Choudhari  
 Quality Manager

AE/RFT-50

## CALIBRATION CERTIFICATE

|                                                                                                                                         |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
|-----------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------|-----------------------|------------------|
| Calibration On<br>18.Oct.2025                                                                                                           | Next Calibration Due<br>17.Oct.2026 | Certificate No.<br>AE/WM/25/10/1473                                                                                                                                                                                              | Certi. Issue Date<br>24.Oct.2025 | Sheet No.<br>01 of 01 |                  |
| M/s Apex Buildsys Limited.<br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur.                                                |                                     | CUSTOMER REFERENCE                                                                                                                                                                                                               |                                  |                       |                  |
|                                                                                                                                         |                                     | SRF No : ACIPL/JC/25-26/883                                                                                                                                                                                                      |                                  |                       |                  |
|                                                                                                                                         |                                     | Gate Pass No. : -                                                                                                                                                                                                                |                                  |                       |                  |
|                                                                                                                                         |                                     | Date of Receipt : 18.Oct.2025                                                                                                                                                                                                    |                                  |                       |                  |
| Order Inward No.                                                                                                                        | ACIPL/25-ISO/10/883/A-158           | Location of Calibration : Onsite                                                                                                                                                                                                 |                                  |                       |                  |
| 01 Description & Identification :                                                                                                       |                                     | UUC : Digital Arc Welding Machine<br>Make : Ador<br>Model No. : CHAMP-600<br>Serial No. : 79/23116709<br>ID. No. : MEC-233<br>Range : 0 to 600 Amp & 0 to 44 Volt<br>Least Count : 1 Amp & 0.1 Volt                              |                                  |                       |                  |
| 02 .                                                                                                                                    |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| SI NO.                                                                                                                                  | DESCRIPTION                         | SR.NO.                                                                                                                                                                                                                           | TRACEBILITY                      | VALIDITY              | CERTIFICATE NO.  |
| 01                                                                                                                                      | Clamp Meter                         | 2408077674                                                                                                                                                                                                                       | NABL CC - 2632                   | 19.May.2026           | AE/CC/25-26/3349 |
| 03 Calibration Procedure reference                                                                                                      |                                     | AE / DFT / 02 - CM/ET/06/08                                                                                                                                                                                                      |                                  |                       |                  |
| 04 Environmental Conditions                                                                                                             |                                     | Temperature at 27.5 °C & 45 to 75 % RH                                                                                                                                                                                           |                                  |                       |                  |
| 05 Calibration Result in Volts. (Observed value is mean of Five reading)                                                                |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| SI No.                                                                                                                                  | Range                               | Observe on Master                                                                                                                                                                                                                | Observe on UUC                   | Deviation             |                  |
| 01                                                                                                                                      | 20                                  | 20.28                                                                                                                                                                                                                            | 20.5                             | 0.22                  |                  |
| 02                                                                                                                                      | 30                                  | 30.35                                                                                                                                                                                                                            | 30.8                             | 0.45                  |                  |
| 03                                                                                                                                      | 40                                  | 40.3                                                                                                                                                                                                                             | 41.2                             | 0.9                   |                  |
| Calibration Result in Amp. (Observed value is mean of Five reading)                                                                     |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| SI No.                                                                                                                                  | Range                               | Observe on Master                                                                                                                                                                                                                | Observe on UUC                   | Deviation             |                  |
| 01                                                                                                                                      | 200                                 | 200.4                                                                                                                                                                                                                            | 200                              | -0.4                  |                  |
| 02                                                                                                                                      | 400                                 | 400                                                                                                                                                                                                                              | 401                              | 1                     |                  |
| 03                                                                                                                                      | 500                                 | 500                                                                                                                                                                                                                              | 502                              | 2                     |                  |
| 04                                                                                                                                      | 600                                 | 600                                                                                                                                                                                                                              | 600                              | 0                     |                  |
| 06 Remarks                                                                                                                              |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| 01.This certificate issued as per customer requirment.                                                                                  |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| 02.UUC = Unit Under Calibration.                                                                                                        |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| 03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.                |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| **** End of Certificate ****                                                                                                            |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |
| <br>Calibrated By<br>Y. P. Mute<br>Calibration Engg. |                                     |  <br>Authorised By<br>A. S. Choudhari<br>Quality Manager |                                  |                       |                  |
| AE/RFT-50                                                                                                                               |                                     |                                                                                                                                                                                                                                  |                                  |                       |                  |

## CALIBRATION CERTIFICATE

|                |                      |                  |                   |           |
|----------------|----------------------|------------------|-------------------|-----------|
| Calibration On | Next Calibration Due | Certificate No.  | Certi. Issue Date | Sheet No. |
| 18.Oct.2025    | 17.Oct.2026          | AE/WM/25/10/1474 | 24.Oct.2025       | 01 of 01  |

|                                                                                                 |                           |                         |          |
|-------------------------------------------------------------------------------------------------|---------------------------|-------------------------|----------|
| <b>M/s Apex Buildsys Limited.</b><br>Plot No - D3, MIDC Industrial Area,<br>Umred, Dist-Nagpur. | <b>CUSTOMER REFERENCE</b> |                         |          |
|                                                                                                 | SRF No                    | : ACIPL/JC/25-26/883    |          |
|                                                                                                 | Gate Pass No.             | : -                     |          |
|                                                                                                 | Date of Receipt           | : 18.Oct.2025           |          |
| Order Inward No.                                                                                | ACIPL/25-ISO/10/883/A-159 | Location of Calibration | : Onsite |

**01 Description & Identification :**

|             |                               |
|-------------|-------------------------------|
| UUC         | : Digital Arc Welding Machine |
| Make        | : Ador                        |
| Model No.   | : CHAMP-600                   |
| Serial No.  | : 79/23116712                 |
| ID. No.     | : MEC-231                     |
| Range       | : 0 to 600 Amp & 0 to 44 Volt |
| Least Count | : 1 Amp & 0.1 Volt            |

**02 .**

| SI NO. | DESCRIPTION | SR.NO.     | TRACEBILITY    | VALIDITY    | CERTIFICATE NO.  |
|--------|-------------|------------|----------------|-------------|------------------|
| 01     | Clamp Meter | 2408077674 | NABL CC - 2632 | 19.May.2026 | AE/CC/25-26/3349 |

**03 Calibration Procedure reference** AE / DFT / 02 - CM/ET/06/08

**04 Environmental Conditions** Temperature at 27.5 °C & 45 to 75 % RH

**05 Calibration Result in Volts. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 20    | 19.87             | 20.3           | 0.43      |
| 02     | 30    | 29.82             | 30.5           | 0.68      |
| 03     | 40    | 39.5              | 40.8           | 1.3       |

**Calibration Result in Amp. (Observed value is mean of Five reading)**

| SI No. | Range | Observe on Master | Observe on UUC | Deviation |
|--------|-------|-------------------|----------------|-----------|
| 01     | 200   | 199.2             | 200            | 0.8       |
| 02     | 400   | 400               | 401            | 1         |
| 03     | 500   | 500               | 501            | 1         |
| 04     | 600   | 600               | 602            | 2         |

**06 Remarks**


01.This certificate issued as per customer requirment.

02.UUC = Unit Under Calibration.

03.The Standards used for calibration are tracebel to National / International Standard through accredited Laboratories.

\*\*\*\* End of Certificate \*\*\*\*

  
 Calibrated By  
 Y. P. Mute  
 Calibration Engg.



  
 Authorised By  
 A. S. Choudhari  
 Quality Manager

AE/RFT-50